


Data file: E:\CHEM32\DATA\201217\602511 20110077Final.D
 Sample name: 602511 20110077Final
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 25-35% in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A (A-006)
 Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 53
 Injection date: 2020/12/17 13:34:42 Injection: 1 of 1
 Last changed: 2020/12/17 15:36:09 Injection volume: 10.000
 Acq.operator: QC

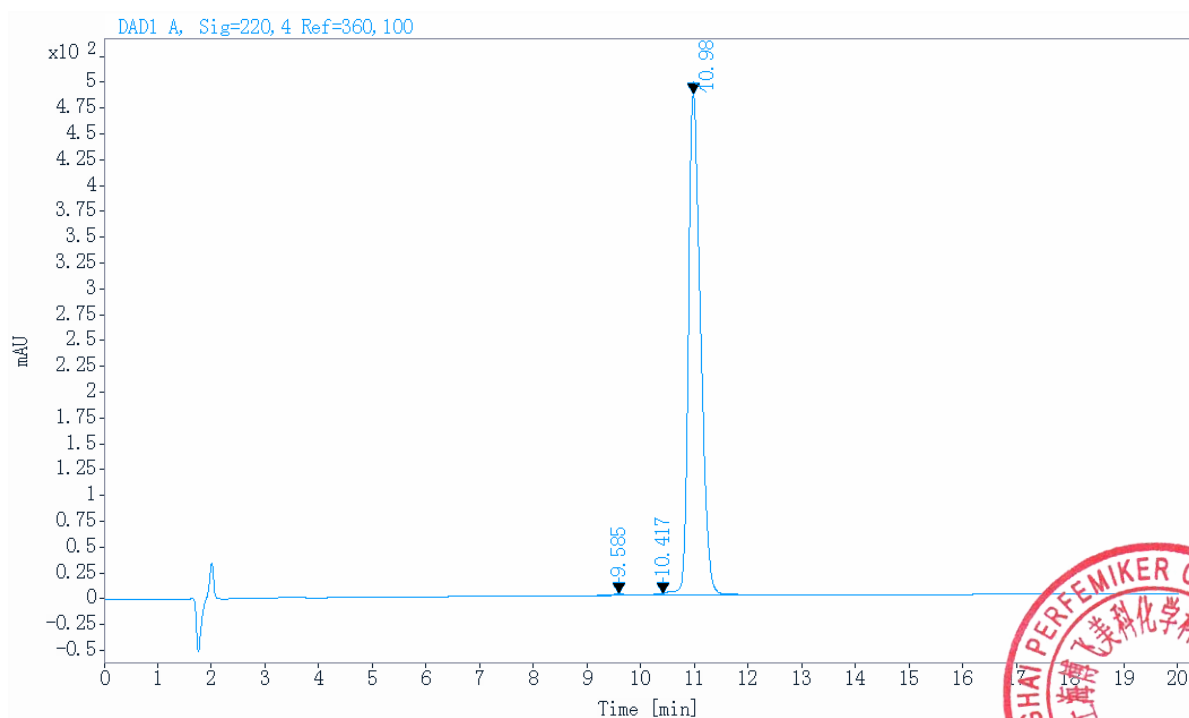

Signal: DAD1 A, Sig=220,4 Ref=360,100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
9.585	BB	0.2517	33.3692	1.9302	0.4335	
10.417	MF	0.2151	22.8383	1.7694	0.2967	
10.980	FM	0.2622	7641.0972	485.6340	99.2698	
Sum			7697.3047			